


The BD Veritor™ System Flu A+B Meets the New FDA Requirements to Assure Safety and Effectiveness for Rapid Influenza Antigen Detection Tests (RIDTs)

 **CLASS II**

A **digital immunoassay** with performance that meets the new FDA Class II requirements for RIDTs


+81 INFLUENZA STRAINS
Offers a broad range of detection

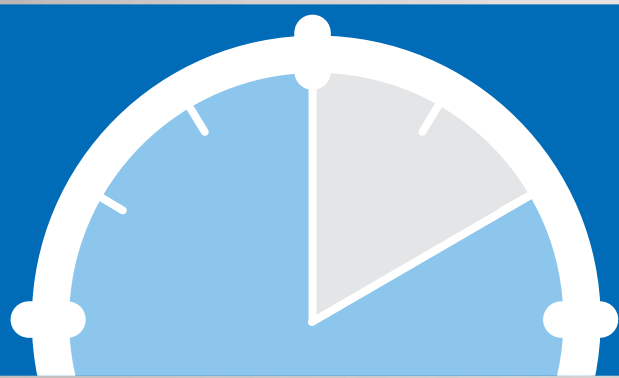

Objective and accurate results in under 11 minutes

>17,000 Instruments placed and used in hospitals, outpatient and point-of-care settings

First Clinical Laboratory Improvement Amendment (CLIA) waived digital immunoassay (DIA) that allows rapid detection of flu

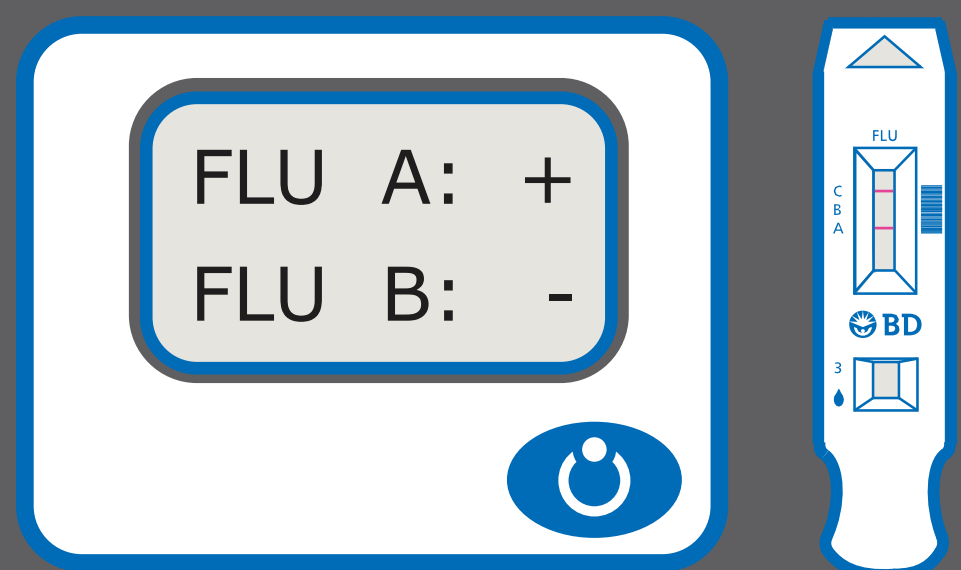

BD, BD Logo and BD Veritor are trademarks of Becton, Dickinson and Company

©2017 BD January 2017
Printed in USA



BD Diagnostics
7 Loveton Circle
Sparks, MD
21152-0999
800.638.8663
www.bd.com/ds