

Pediatric StO₂ Accuracy Verification of ForeSight Jr NIRS Tissue Oximetry System

Scope

This review describes the accuracy verification method and resultant performance for monitoring near-infrared spectroscopy (NIRS) tissue oxygen saturation (StO₂) of the ForeSight Jr sensor on cerebral and somatic body sites

Background

Two separate internal review board (IRB) approved protocols were undertaken in multiple institutions to gather StO₂ data from pediatric patients with a range of age, weight, ethnicity, and varied skin tones. The study enrolled children undergoing cath lab procedures or babies in the NICU, rather than healthy volunteers (as used in the StO₂ accuracy verification of adults per the ISO-2021 StO₂ device standard¹), as it would pose safety and ethical concerns to healthy neonatal patients.

ForeSight Jr sensors emit 5 wavelengths of near-infrared light (685, 730, 770, 810, and 870 nm) and each contain two detectors purposefully placed at 12 mm and 40 mm from the light source for medium sensors and 9 mm and 25 mm for small sensors, which results in a deep detector penetration of 2.0 and 1.25 cm, respectively. The component spacing is used to separate superficial tissue from the StO₂ for the tissue of interest. The ForeSight algorithm evaluates the detected light to compensate for background tissue light absorption and scattering, as well as skin pigmentation, to derive an accurate StO₂.²

Medium and Small Sensors

Medium sensor – Cath-Lab protocol to verify StO₂ accuracy in subjects ≥ 2.5 kg

The medium sensor research protocol was for pediatric patients undergoing cardiac catheterization at three university teaching hospitals in the United States.

These patients had two sensors on their forehead to measure cerebral StO₂ and sensors over their lower abdomen and posterior flank. The subject's weight determined the size of the sensors used as per the device intended use. As in prior verification studies,^{3,4} these StO₂ values were compared with an arteriovenous blood reference derived from arterial (SaO₂) and venous samples from multiple locations. All blood specimens were sampled at the same time as the StO₂ measurement and analyzed with a CO-oximeter for functional oxygen saturation.

For both the cerebral and somatic StO₂ data, the arterial blood specimens were from the aorta or femoral artery. The venous blood sample locations matched the tissue of interest, for cerebral and somatic measurements. For the cerebral StO₂, the catheter was placed in the jugular vein (SjvO₂ blood specimen) for the cerebral StO₂ and in a central venous location for the somatic measurement. Because of the varied types of congenital heart disease in the subject pool, the selected somatic sampling site for each subject was based upon a location unaffected by their particular disease. Thus, the sampling sites included the inferior vena cava (IVC), superior vena cava, right atrium, right ventricle, left pulmonary artery and/or the right pulmonary artery.

The weighted arteriovenous blood reference for StO₂ was based on the assumption that 70% of blood in both cerebral and somatic tissues is venous, while 30% is arterial.^{5,6} The SjvO₂ blood represents venous blood in the brain, whereas the selected venous location was representative of the somatic tissues of interest.

Small Sensor – NICU protocol to verify StO₂ accuracy in subjects ≤ 5 kg

This research protocol enrolled ≤ 5 kg patients in the NICUs of 6 prestigious hospitals in the United States. An inclusion criterion was an umbilical venous catheter for routine care, which was the source for the protocol's SvO₂ blood samples for the somatic StO₂ accuracy verification.

To verify accuracy of cerebral StO₂ with a small sensor, the ForeSight Jr system was directly compared with the predicate FDA-cleared ForeSight system.⁷ Unlike the other ForeSight system accuracy verification studies, this cerebral study did not include SjvO₂ blood specimens, because insertion of an internal jugular venous catheter is not routine in neonates. A small ForeSight Jr sensor was placed on the subject's forehead for 2 minutes, followed by a predicate small ForeSight sensor (reference) for 2 minutes. This sequence was repeated once for each subject (with all sensors applied in the same position on round-two).



To verify accuracy of somatic StO₂, a small sensor was placed for 2 minutes on the posterior-flank and then, for 2 minutes on each of 6 anterior abdomen locations (left & right flank, liver, and over the right-lower, left-lower, and mid-lower quadrants). The venous blood reference was from the umbilical vein catheter and SpO₂ was used for the arterial blood arteriovenous reference, to avoid unnecessary arterial cannulation or blood samples outside of routine care. Blood from the IVC positioned catheter, represents venous blood to the somatic sites in these small patients.

The results from the arteriovenous reference were compared with ForeSight sensor StO₂ values to derive the bias and precision. The medium sensor analysis used data only from the Cath-Lab protocol, while the small sensor analysis combined values from both the Cath-Lab and NICU protocols.

Results

The medium sensor was applied to subjects of balanced gender and various ethnicity (African American, American Indian, Asian, Caucasian, and Hispanic). The patient age and weight ranges were 0.1 to 16.7 years and 3.3 to 73.3 kg, respectively. The medium sensor had an StO₂ bias and precision (at 1 standard deviation) of 0.97 ± 5.43% (n=72) for the cerebral site, and -0.14 ± 5.75% (n=67) for somatic sites (see Figures 1 & 2). The range of StO₂ values for cerebral and somatic sites were across a wide range of saturations (Table 1).

The small sensor was applied to subjects of balanced gender and various ethnicity (African American, American Indian, Asian, Caucasian, and Hispanic). The patient age and weight ranges were 1 to 317 days and 0.5 to 7.7 kg, respectively. The small sensor had an StO₂ bias and precision (at 1 standard deviation) of -0.74 ± 5.98% (n=73) and 2.35 ± 5.25% (n=54) for the somatic sites (Figures 3 & 4). The range of StO₂ values for cerebral and somatic were across a wide range of saturations (Table 1).

Discussion

There are multiple facets in accuracy performance testing that likely improved performance (and what was the rationale of each).

- 1 Use of the ISO 80601-2-85:2021 standard for performance of cerebral tissue oximeter equipment¹ (i.e., the reference for StO₂ is defined in the standard and used as part of regulatory submissions)
- 2 The sensor emitter and detectors are spaced specifically

for each size sensor to match the target tissue depth by patient size (i.e., the target tissue of interest is interrogated to derive StO₂, while correcting for superficial tissues)⁸

- 3 Accuracy performance data were from pediatric patients, representing the population of intended use (i.e., assuring the verified performance was demonstrated over a range of patient age, weight, and ethnicity with varied skin tones)²

At the time of this publication, we are unaware of another NIRS manufacturer with compliance to the 2021 ISO standard, the volume and breath of tested pediatric patients, or the tight precision of accuracy performance.

Conclusions

The ForeSight Jr system with medium and small sensors demonstrated high accuracy in a broad sampling of pediatric age, weight, and ethnicity with varied skin tones. Per the FDA cleared indications for use, the ForeSight system can accurately determine cerebral and somatic StO₂ values on any age child via a range of sensor sizes.⁸ As of this writing, no other NIRS manufacturer has claimed conformance to the ISO standard for accuracy performance in children.

Sensor Size	Body Site	Wt. Range (IFU)	Accuracy (bias ± precision @ 1sd)	StO ₂ Test Range
Medium	Cerebral	≥ 3 kg	0.97 ± 5.43	44 to 91%
Medium	Somatic	≥ 3 kg	-0.14 ± 5.75	52 to 88%
Small	Cerebral	< 8 kg	-0.74 ± 5.98	44 to 90%
Small	Somatic	< 5 kg	2.35 ± 5.25	66 to 96%

Table 1: Summary of ForeSight Jr system accuracy validation findings with indications for use of sensors

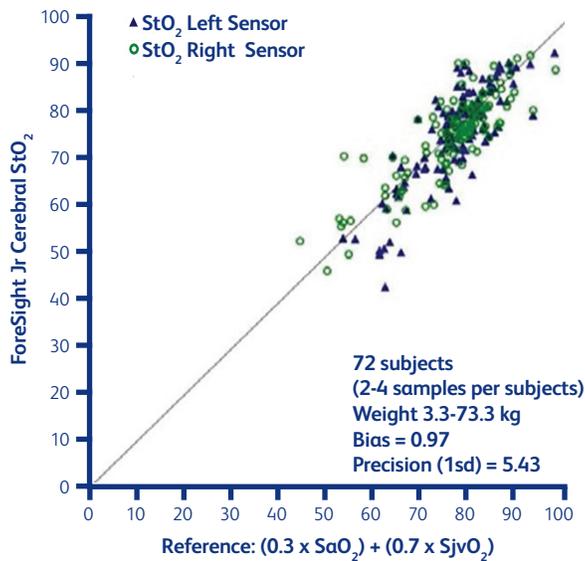


Figure 1: StO₂ vs Reference with medium ForeSight Jr sensor on cerebral sites

Each blue triangle is the left-forehead StO₂ value linked to the simultaneous set of SaO₂ and SjvO₂ blood samples. Each green circle is the right-forehead StO₂ value linked to a simultaneous set of SaO₂ and SjvO₂ blood samples.

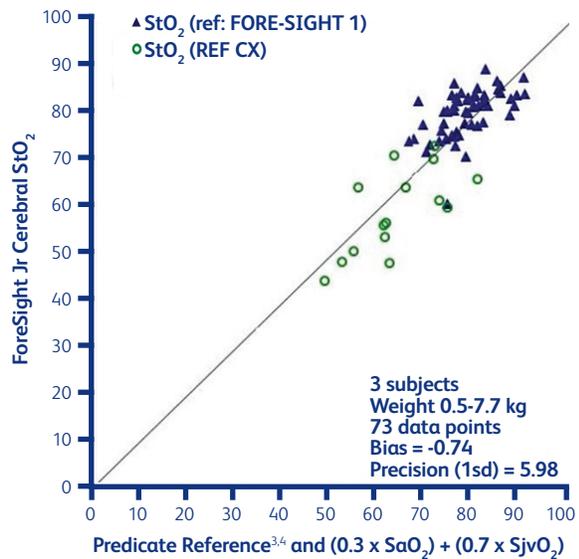


Figure 3: StO₂ vs Reference with small ForeSight Jr sensor on cerebral sites

Each blue triangle is the StO₂ value linked the predicate reference, and the green circles are each simultaneous set of predicate SaO₂ and SjvO₂ blood samples.

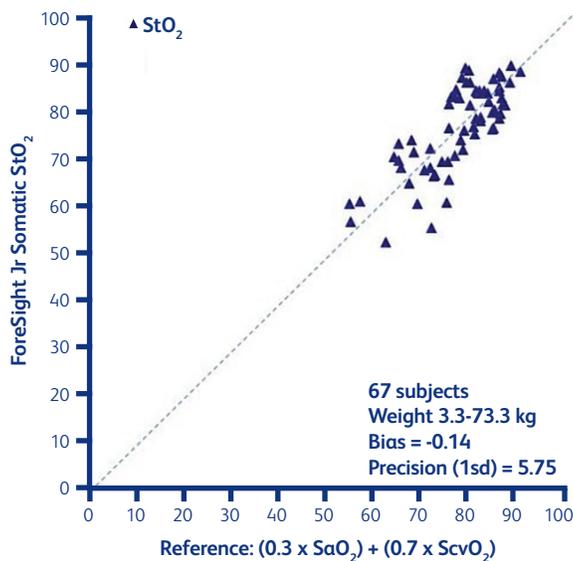


Figure 2: StO₂ vs Reference with medium ForeSight Jr somatic sensor

Each blue triangle is the StO₂ value linked to a simultaneous set of SaO₂ and venous ScvO₂ blood samples.

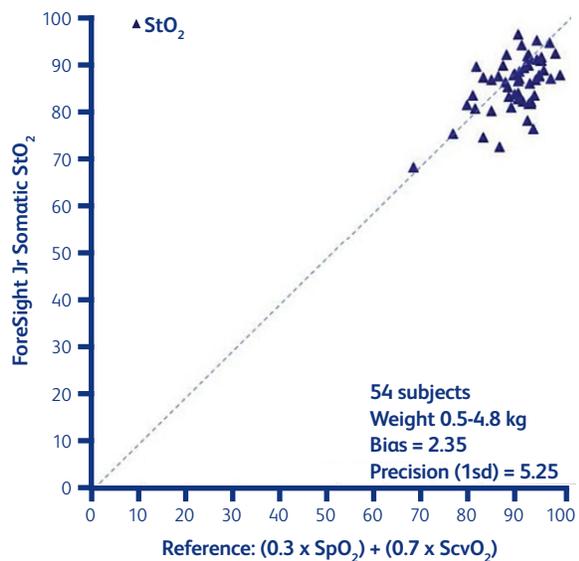


Figure 4: StO₂ vs Reference with small ForeSight Jr sensor on somatic sites

Each blue triangle is the StO₂ value linked to a simultaneous set of SpO₂ and venous ScvO₂ blood sample values.

References

- 1 ISO 80601-2-85:2021. Medical electrical equipment — Part 2-85: Particular requirements for the basic safety and essential performance of cerebral tissue oximeter equipment. [Annex EE: (human subjects) controlled desaturation study for the verification of StO₂ accuracy of cerebral tissue oximeter equipment]
- 2 Benni PB. CAS Medical Systems, Inc., assignee. Method for spectrophotometric blood oxygenation monitoring. United States patent US 8923943. 2014 Dec 30.
- 3 Benni PB, Chen B, Dykes FD, Wagoner SF, Heard M, Tanner AJ, Young TL, Rais-Bahrami K, Rivera O, Short BL. Validation of the CAS neonatal NIRS system by monitoring vv-ECMO patients: preliminary results. *Adv Exp Med Biol*. 2005;566:195-201.
- 4 Rais-Bahrami K, Rivera O, Short BL. Validation of a noninvasive neonatal optical cerebral oximeter in veno-venous ECMO patients with a cephalad catheter. *J Perinatol*. 2006;26(10):628-35.
- 5 Ito H, Kanno I, Iida H, Hatazawa J, Shimosegawa E, Tamura H, Okudera T. Arterial fraction of cerebral blood volume in humans measured by positron emission tomography. *Ann Nucl Med*. 2001;15(2):111-6.
- 6 Pang CC. Measurement of body venous tone. *J Pharmacol Toxicol Methods*. 2000;44(2):341-60.
- 7 FDA 510(k) summary for K061960. FORE-SIGHT Cerebral Oximeter Monitor. CAS Medical System, Inc. United States Food and Drug Administration. 2006 Sep 05.
- 8 Ferrari M, Mottola L, Quaresima V. Principles, techniques, and limitations of near infrared spectroscopy. *Can J Appl Physiol*. 2004;29(4):463-87.
- 9 FDA 510(k) summary for K213682. HemoSphere Advanced Monitor with ForeSight Oximeter Cable. Edwards Lifesciences LLC. United States Food and Drug Administration. 2022 Jun 22.

CAUTION: Federal (United States) law restricts these devices to sale by or on the order of a physician. See instructions for use for full prescribing information, including indications, contraindications, warnings, precautions and adverse events.

BD, Irvine, CA 92618 USA

[bd.com](https://www.bd.com)

BD, the BD Logo, ForeSight and ForeSight Jr are trademarks of Becton, Dickinson and Company or its affiliates. All other trademarks are the property of their respective owners. © 2026 BD. All rights reserved. BD-149630 v1.0 US

